

**McKesson**

# Standard and Fiberoptic Laryngoscope Blades/Handles

## INSTRUCTIONS FOR USE

Thank you for choosing a McKesson laryngoscope.

## DEVICE DESCRIPTION AND INTENDED USE

A laryngoscope is a two-part, handheld device consisting of a handle that contains batteries and a detachable blade. Laryngoscopes are designed to provide illumination within the larynx during the process of performing intubations. This instruction book covers standard, fiberoptic type and disposable laryngoscopes. Fiberoptic laryngoscopes are indicated by an "F" following the item number.

## CONTRAINDICATIONS

The following are only relative contraindication to tracheal intubation:

1. Severe airway trauma or obstruction that does not permit safe passage of an endotracheal tube. Emergency cricothyrotomy is indicated in such cases.
2. Cervical spine injury, in which the need for complete immobilization of the cervical spine makes endotracheal intubation difficult.

## GENERAL WARNINGS

**A warning statement in this manual identifies a condition or practice which, if not corrected or discontinued immediately, could lead to patient injury, illness, or death.**

**WARNING:** Federal law restricts this device to sale by or on the order of a physician or licensed healthcare practitioner.

**WARNING:** ONLY TRAINED PERSONNEL SHOULD USE A LARYNGOSCOPE FOR INTUBATION.

**WARNING:** It is recommended that spare lamps, batteries, and replacement parts always be available for emergency use.


**WARNING:** The sterilization guidelines included in this instruction booklet are intended as procedures compatible with specific materials. Sterilization must be performed to approved hospital protocol. There is no guarantee that any of the recommended methods will guarantee sterility. This must be validated by the hospital and/or sterilization equipment manufacturer.

**WARNING:** Fiberoptic handles may be used with ALL fiberoptic blades (reusable or disposable) that conform to the ISO 7376 standards. Standard handles may be used with any standard blades that conform to the ISO 7376 standards. Standard and fiberoptic blades and handles are NOT interchangeable.

## OPERATION OF ALL LARYNGOSCOPE MODELS

**To Activate:** Attach selected blade onto handle by hooking blade onto handle rod as shown in Figure 1. Pull blade upward to open position to automatically activate light.

To turn off, push blade downward into off position and disconnect from handle. (See Figure 1).



## COMPATIBILITY/STANDARDS

Standard McKesson laryngoscopes conform to current ISO 7376 standards. They are compatible with virtually all major brands of standard illumination hook-on blades and handles.

Fiberoptic McKesson laryngoscope blades conform to current ISO 7376 standards. They are compatible with virtually all major brands of fiberoptic illumination hook-on blades and handles. For easy visual identification, ALL fiberoptic models are clearly delineated by a green indicator on both handle and blade.

## CLEANING, DISINFECTING, AND STERILIZATION PROCEDURES

McKesson laryngoscope blades are crafted from rugged stainless steel. Reusable handles are machined from chrome-plated brass or anodized aluminum. To ensure maximum life and optimum performance, the following instructions should be strictly followed.

See the sections on the reverse panel for specific cleaning, disinfection, and sterilization procedures for your laryngoscope type.

### Cleaning Procedure (All Reusable Models)

Almost immediately after use, laryngoscope blades should be cleaned to prevent blood, saliva etc. residues from drying. On Conventional blades, the lamp socket and wires are an integral part of the blade for cleaning and replacement.

**WARNING:** Ultrasonic cleaning is not recommended.

### Disinfection/Sterilization Warnings for All Laryngoscope Blades

**CAUTION:** Laryngoscope blades do not come sterilized. The Sterrad process is NOT to be used with disposable fiberoptic blades or reusable fiberoptic blades.

**WARNING:** Flash autoclaving and hot air sterilization are not recommended; these processes will damage the instrument. The repeated high temperature and changes in temperature caused by autoclaving will shorten the life of all laryngoscope products.

**WARNING:** Do not immerse blades in bleach, Betadine, or peroxide solutions.

Doing so will severely damage the instrument. Also, avoid metal-to-metal contact on non-disposable blades.

### Disinfection/Sterilization Warnings for All Battery Handles

**CAUTION:** Do not allow excess fluid to seep into electrical contact. Be sure that the top and bottom of the battery handle are secure before use. Poor maintenance of this device or failure to follow the warnings in this instruction booklet could result in device failure and/or patient injury. **NOTE:** Remove lamp cartridge, bulb, and batteries before disinfecting/sterilizing.

### Basic Cleaning Procedure for Standard and Fiberoptic Blades

Prepare a Klenzyme®, Manu-klenz™, or equivalent cleaning solution as per the manufacturer's instructions and soak for ten minutes. Rinse devices with lukewarm running tap water for one minute to remove any residual detergent after cleaning. Dry with a clean, lint-free cloth.

**McKesson**

Questions? Call 1-800-777-4908

### Satisfaction Guaranteed

If you are not completely satisfied with any McKesson Brands product, you may return it for a full refund or credit.

Distributed by McKesson Medical-Surgical Inc.  
Richmond, VA 23233  
PVN A0918  
Made in Pakistan

### Basic Cleaning Procedures for Standard and Fiberoptic Handles

Prepare a Klenszyme®, Manu-klenz™, or equivalent cleaning solution as per the manufacturer's instructions. Remove both end caps, lamp cartridge and bulb, and batteries from device, and rinse with lukewarm tap water until all visible contamination has been removed. Soak handle and end caps in the prepared solution for a minimum of ten minutes, ensuring that all components are fully submerged. After the soak, the components should be scrubbed with a soft bristled brush paying particular attention to hard to reach areas. Rinse with cool running tap water to remove all residual detergent. Dry with a clean, lint free cloth. Note: Always allow handles to completely dry before disinfection or use. Lamp cartridge and bulb can be wiped with a cloth dampened with 70% isopropyl alcohol. DO NOT ALLOW SOLUTION TO ENTER INTO THE CARTRIDGE. The lamp cartridge and bulb CANNOT be SOAKED OR AUTOCLAVED.

### High Level Disinfection for Standard and Fiberoptic Blades

To achieve high level disinfection, a 2.4% glutaraldehyde solution (Cidex® or equivalent) must be prepared at 77°F (25°C) to the manufacturer's instructions. The blades should be fully immersed in the disinfectant for a minimum of 45 minutes. No air bubbles should be visible on the immersed blades during this soak time. The blades should then be removed from the disinfectant and immersed in purified water to rinse off all disinfectant. Immersion should be for a minimum of one minute and the process should be repeated two additional times using fresh purified water each time. Once rinsing is complete, the blades should be thoroughly dried using a sterile, lint-free cloth. Note: Always allow blades to completely dry before use.

### High Level Disinfection for Standard and Fiberoptic Handles

To achieve high level disinfection, a 2.4% glutaraldehyde solution (Cidex® or equivalent) must be prepared at 77°F (25°C) to the manufacturer's instructions. The end caps of the handles, lamp cartridge and bulb, and batteries must be removed. Both the end caps and handles should be fully immersed in the disinfectant for a minimum of 45 minutes. No air bubbles should be visible on the immersed components during this soak time. The components should then be removed from the disinfectant and immersed in purified water to rinse off all disinfectant. Immersion should be for a minimum of one minute and the process should be repeated two additional times using fresh purified water each time. Once rinsing is complete, the components should be thoroughly dried using a sterile, lint-free cloth. Note: Always allow components to completely dry before reassembling the handles, inserting batteries, or using the devices. Lamp cartridge and bulb can be wiped with a cloth dampened with 70% isopropyl alcohol. DO NOT ALLOW SOLUTION TO ENTER INTO THE CARTRIDGE. The lamp cartridge and bulb CANNOT be SOAKED OR AUTOCLAVED.

### Steris Sterilization Processes for Disposable and Fiberoptic Laryngoscopes

This product has been validated with the V-PRO 1 Standard Cycle; V-PRO 1 Plus Lumen and Non Lumen Cycles; V-PRO maX Lumen, Non Lumen, and Flexible Cycles; V-PRO 60 Lumen and Non Lumen Cycles using the V-PRO 60 Low Temperature Sterilization System with VAPPROX® HC Sterilant and VPRO maX Low Temperature Sterilization System.

### Steam Sterilization for Standard and Fiberoptic Blades and Handles

Sterilizer Type:	Prevacuum	Sterilizer Type:	Gravity
Preconditioning Pulses:	3	Minimum Temperature:	249.8°F (121°C)
Minimum Temperature:	269.6°F (132°C)	Full Cycle Time:	30 minutes
Full Cycle Time:	4 minutes	Minimum Dry Time:	15 minutes
Minimum Dry Time:	20 minutes		

### REPAIR/MAINTENANCE

#### Battery Replacement: (Reuseable Models)

1. Unscrew bottom cap of handle and remove batteries.
2. Replace with appropriate size battery, taking care to insert positive ends first. Screw bottom cap on and tighten (Figure 2).

**NOTE:** Alkaline batteries should be used with your handle for maximum performance and are recommended for replacement. Ordinary carbon zinc batteries may also be used.

#### Battery Replacement: (4067F Stubby Handle)

1. Unscrew bottom cap of handle and remove battery insert.
2. Replace with appropriate size batteries. Insert 1 battery positive end first and the other negative end first into battery insert, paying attention to the polarity markings. Slide battery insert back into handle following the direction of the "Insert This Way Only" arrows. Screw bottom cap on and tighten (Figure 3).

**NOTE:** Alkaline batteries should be used with your handle for maximum performance and are recommended for replacement. Ordinary carbon zinc batteries may also be used.

#### Lamp Replacement: (Standard Models)

For correct illumination, alignment, and assurance of watertight seal during immersion/autoclave, we recommend using only lamp model 4500-1 and 4501-1 replacement lamps for standard blades.

1. To remove lamp on standard blades, grip lamp collar and rotate lamp counterclockwise until free.
2. Replace the lamp with a new lamp.
3. Verify that lamp is sufficiently tightened before use.

**CAUTION:** Be sure lamp's glass surface is clean and free from fingerprints after assembly. If necessary, the glass may be cleaned with a soft cloth or cotton ball moistened in alcohol.

#### Lamp Replacement: (Fiberoptic Models)

For correct illumination and alignment, we recommend using only replacement lamp model 5111N-4 (Figure 4).

1. Prior to removal, allow lamp time to cool.
2. Unscrew the laryngoscope head from the barrel of the handle in a counterclockwise direction.
3. Pull lamp out of the laryngoscope head. The lamp is friction fit and does not need to be twisted.
4. Insert replacement lamp by firmly pressing into head until it is completely seated.
5. Screw the laryngoscope head onto the barrel of the handle. Tighten by hand only.

**CAUTION:** Be sure lamp's glass surface is clean and free from fingerprints after assembly. If necessary, the glass may be cleaned with a soft cloth or cotton ball moistened in alcohol.

### Fiberoptic Light Guide Replacement

1. Loosen the locking screw with a screwdriver. (Note: This screw is NOT designed to be completely removed. This prevents the screw from falling out while the laryngoscope is in use. DO NOT attempt to remove this screw from the laryngoscope blade.)
2. Pull out the green base of the fiberoptic bundle and slide out the light guide (Figure 5). (Note: The fiberoptic bundle is tightly fitted and may be difficult to remove.)
3. Insert new fiberoptic bundle by reversing the above steps.
4. Tighten the locking screw, ensuring that the fiberoptic bundle is securely attached to the laryngoscope blade.




Figure 5

### TEST PROCEDURES

Laryngoscope blades and handles should always be tested after cleaning/disinfecting/sterilization, and prior to use. To test, connect the laryngoscope blade to handle and push blade to ON position. If the unit fails to light or flickers, check the lamp for a secure connection, batteries, and electrical contacts. Be sure to have adequate supplies of replacement bulbs and batteries. Caps on battery handle should be secure before use. If they are not, it could cause the blade to move out of position. Laryngoscopes should be visually inspected for wear or aging prior to use and after long storage periods. It is strongly recommended that back-up laryngoscopes are kept on hand for emergency situations.

### REPLACEMENT PARTS CHART

DESCRIPTIONS	STANDARD MODELS	
Laryngoscope Item	Standard Blade	Standard Replacement Lamp
Mac 0	4070	4500
Mac 1	4071	4500
Mac 2	4072	4500
Mac 3	4073	4501
Mac 4	4074	4501
Miller 00	4080-0	4500
Miller 0	4080	4500
Miller 1	4081	4500
Miller 2	4082	4501
Miller 3	4083	4501
Miller 4	4084	4501
Wisconsin 0	4090	4500
Wisconsin 1	4091	4500
Wisconsin 1.5	40915	4500
Wisconsin 2	4092	4501
Wisconsin 3	4093	4501
Wisconsin 4	4094	4501
"C" Cell Handle	4065	N/A
"AA" Cell Handle	4066	N/A
Stubby Handle	4067	N/A

DESCRIPTIONS	FIBEROPTIC MODELS		
Laryngoscope Item	Fiberoptic Blade	Fiberoptic Replacement Lamp	Fiberoptic Light Guide
Mac 0	4070F	N/A	4070FLP-00
Mac 1	4071F	N/A	4071FLP-00
Mac 2	4072F	N/A	4072FLP-00
Mac 3	4073F	N/A	4073FLP-00
Mac 4	4074F	N/A	4074FLP-00
Miller 00	N/A	N/A	N/A
Miller 0	4080F	N/A	4080FLP-00
Miller 1	4081F	N/A	4081FLP-00
Miller 2	4082F	N/A	4082FLP-00
Miller 3	4083F	N/A	4083FLP-00
Miller 4	4084F	N/A	4084FLP-00
Wisconsin 0	N/A	N/A	N/A
Wisconsin 1	N/A	N/A	N/A
Wisconsin 1.5	N/A	N/A	N/A
Wisconsin 2	N/A	N/A	N/A
Wisconsin 3	N/A	N/A	N/A
Wisconsin 4	N/A	N/A	N/A
"C" Cell Handle	4065F	5111N-4	N/A
"AA" Cell Handle	4066F	5111N-4	N/A
Stubby Handle	4067F	5111N-4	N/A




Figure 2

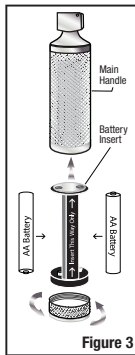


Figure 3




Figure 4