

MCKESSON


Folding Steel Frame Commode

12 qt bucket | heavy duty

For use with MFR#'s 146-11117N-1.

COMMODOE ASSEMBLY INSTRUCTIONS AND PRECAUTIONS


1. Before assembling seat and lid, allow toilet seat and lid to reach room temperature if exposed to cold. This will help prevent the seat and lid clamps from cracking while being assembled onto commode back cross brace.
2. Align the toilet seat clamps onto the back frame rail. (Both clamps should sit outside the pail brackets). Push down on seat until clamps snap firmly into place
3. Repeat the same process for the lid.
4. When removing the seat or lid, always remove lid first and then the seat. To remove, grasp the back of the lid and/or seat and lift.
5. Install commode bucket by dropping into bucket frame. Reverse to remove.

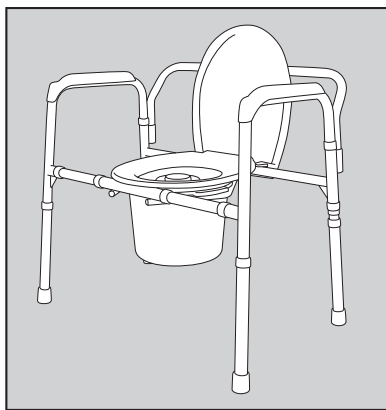

MFR # 146-11117N-1 Shown

WEIGHT CAPACITY: 650 LBS.


FIGURE 1

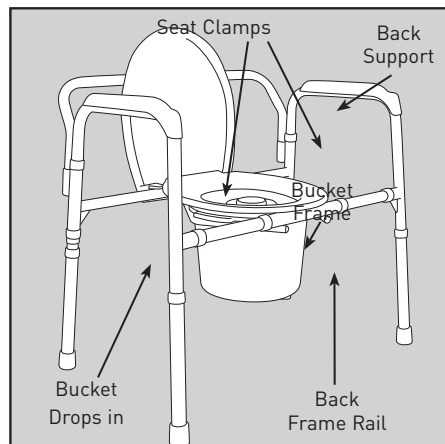

ADJUSTING LEG HEIGHT

1. Before use, adjust height of each leg to your specific needs, making sure all legs are at the same height. When desired height is reached, lock legs into place by aligning buttons into proper holes, per figure 2.
2. To be sure legs are locked into place by pushing down on or by pulling legs.

FIGURE 2

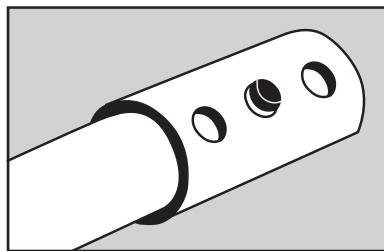

ADDITIONAL PRECAUTIONS

1. Toilet seat must be in down position before use. Failure to do so may result in breakage of commode and possible injury.
2. Do NOT install commode without first reading and understanding this assembly and instruction sheet. If you can not understand these instructions, contact a healthcare, dealer or technical professional before attempting to install. Otherwise, injury or damage may occur.
3. Inspect all parts for shipping damage before assembly. If there is shipping damage - DO NOT USE. Contact dealer/ carrier for further instructions.
4. Make certain that the height adjusting snap buttons fully protrude through the same respective hole of each leg extension. This will ensure that the leg extensions are securely locked in position and an even height is achieved (see Figure 2).
5. Ensure ALL screws, nuts and/or bolts are tightened.
6. Check the rubber tips on the leg extensions for rips, wear or if they are missing. Immediately replace any or all if any of these imperfections exist.
7. All four leg extensions with rubber tips MUST touch the floor simultaneously at all times.
8. Users with limited physical strength should be supervised or assisted while using commode.

Technical support, replacement parts and warranty information? Call 1-866-694-5085. General product questions? Call 1-800-777-4908

Satisfaction Guaranteed

For complete details, please visit
[mms.mckesson.com/mckesson-brands](https://www.mckesson.com/mckesson-brands).

Distributed by McKesson Medical-Surgical Inc.
Richmond, VA 23233
PVN B0518
Made in China